


Appendix 1: Preparing for a Sonography Procedure



HLD = High Level Disinfection; LLD = Low Level Disinfection; Cover = Transducer Cover

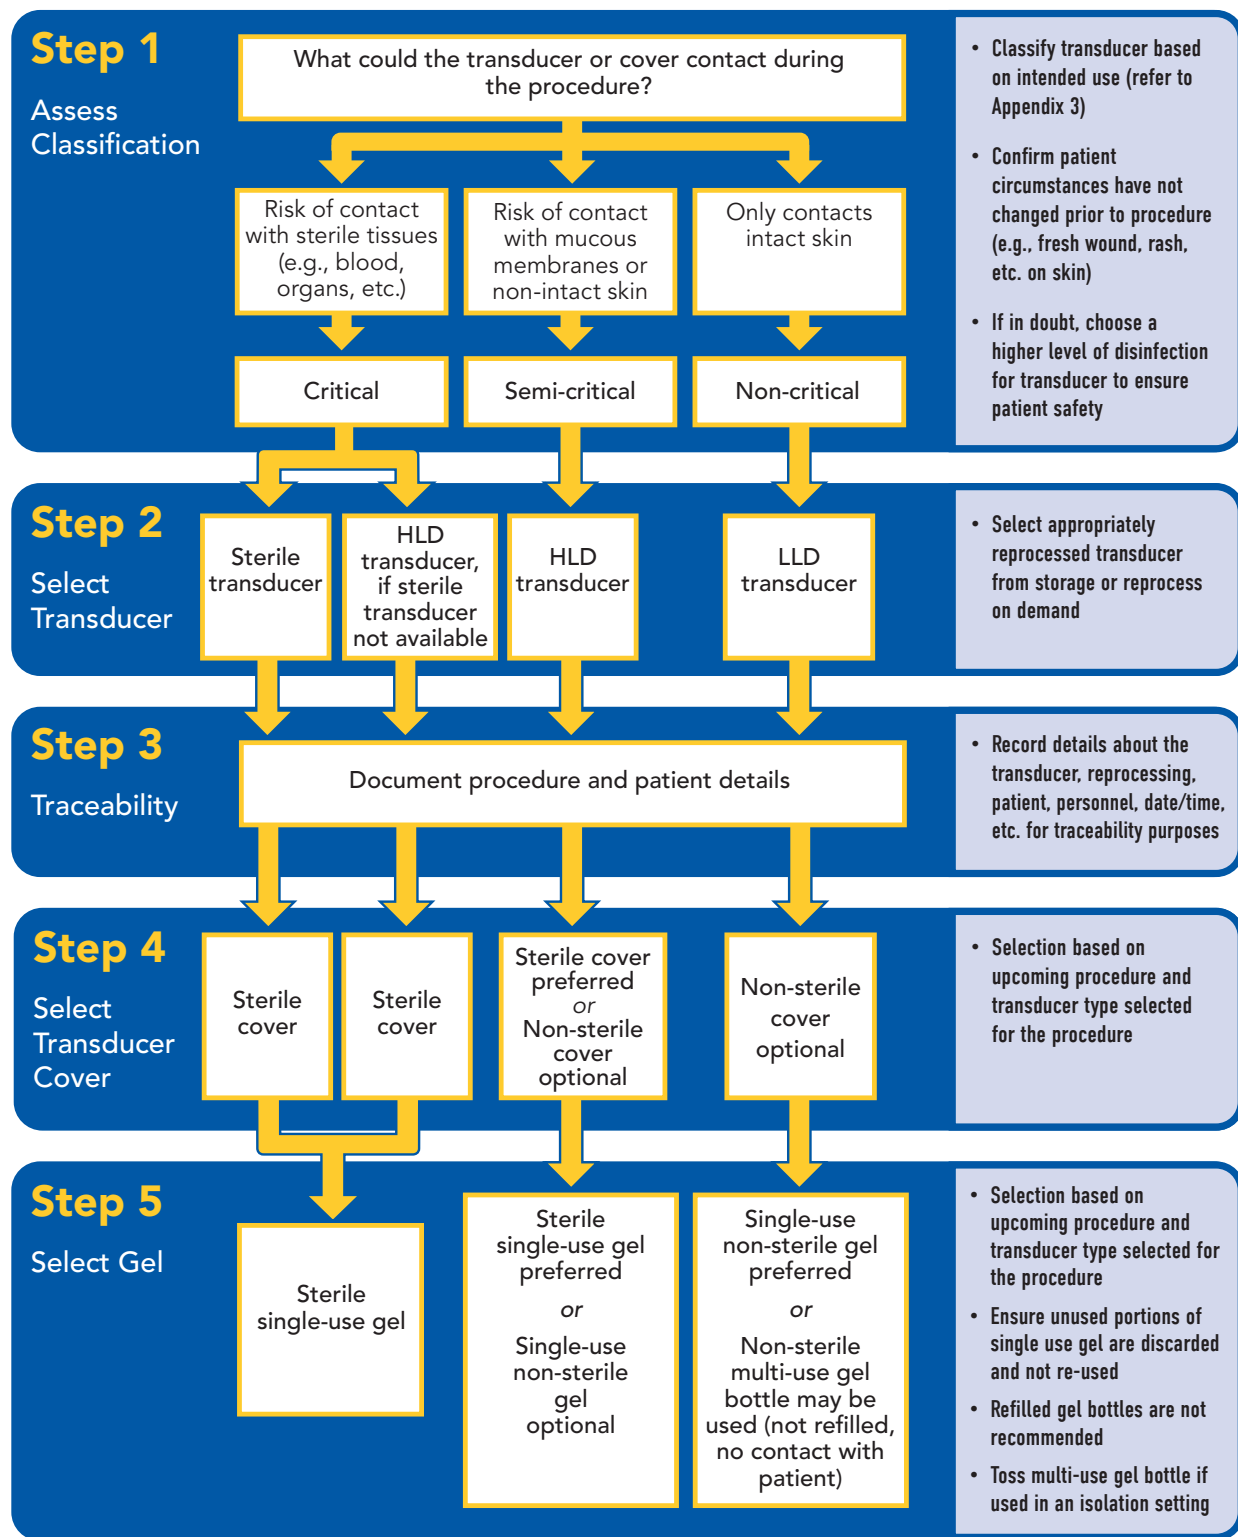