


Appendix 2: Reprocessing the Ultrasound Transducer and Ancillary Equipment

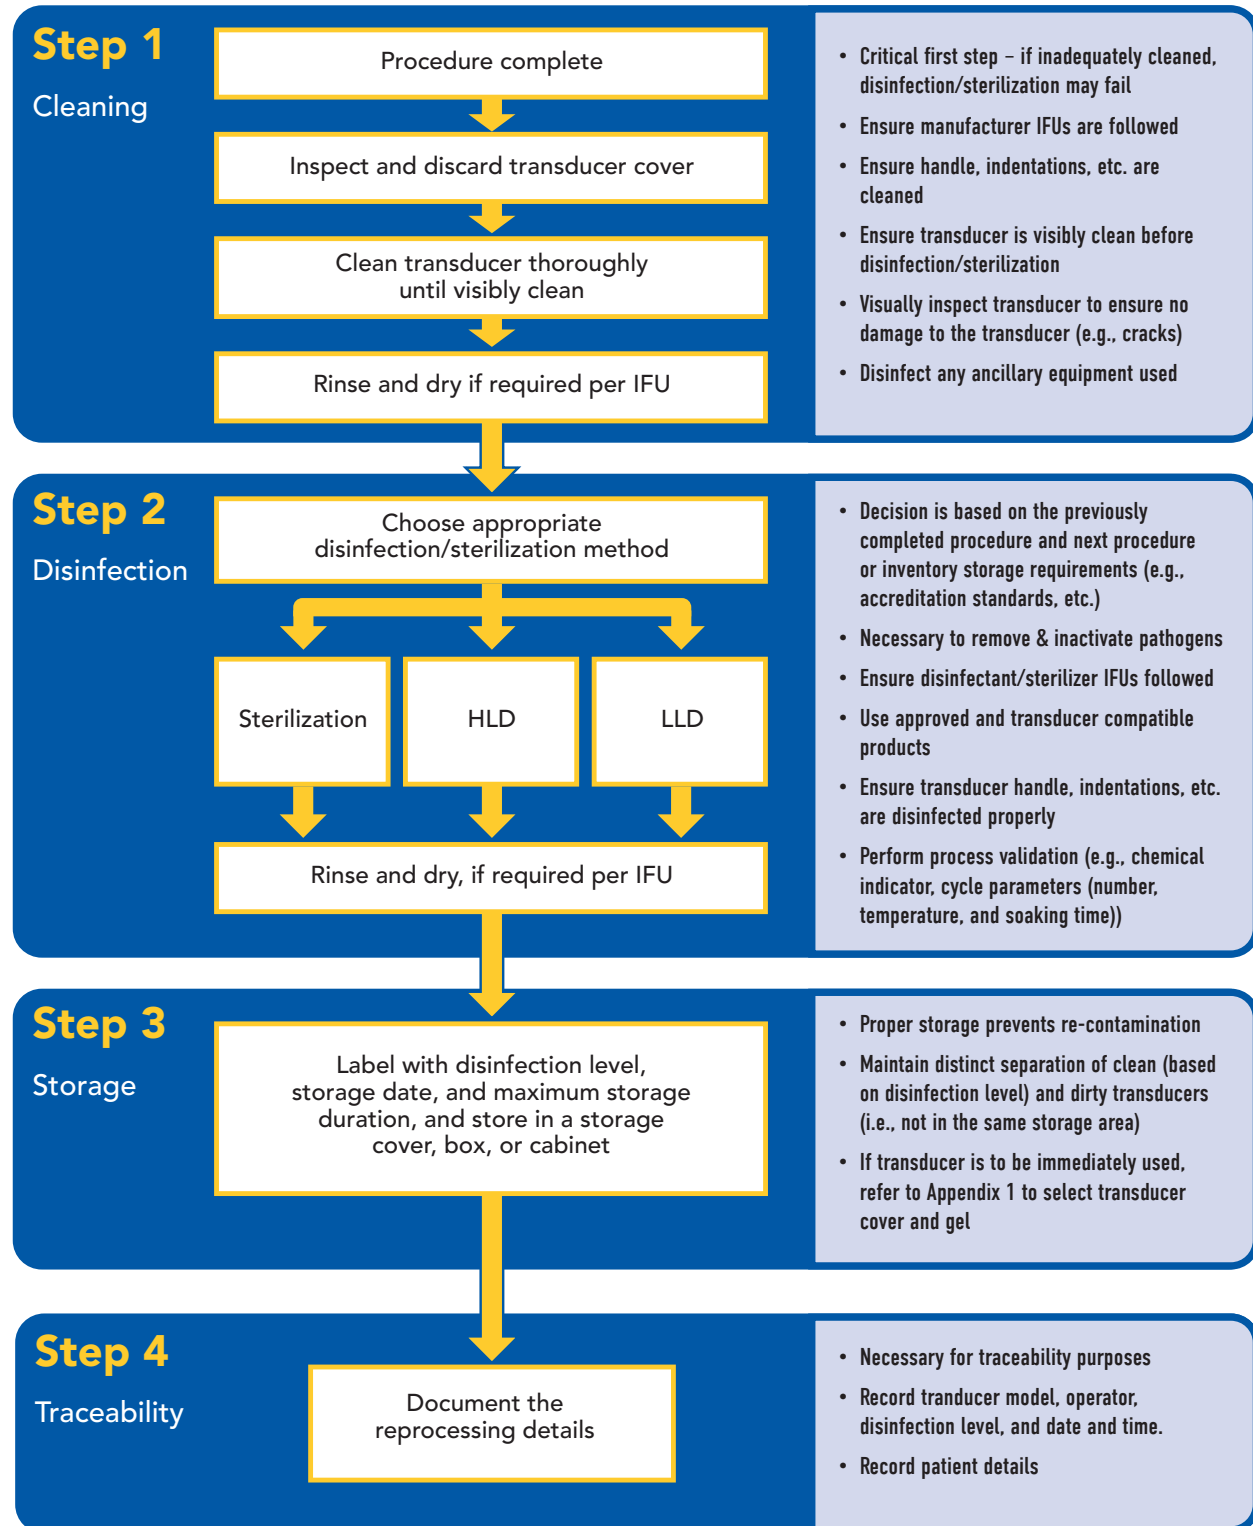

HLD = High Level Disinfection; LLD = Low Level Disinfection; Cover = Transducer Cover; IFU = Instructions for use